



# HTLV BLOT 2.4

## WESTERN BLOT ASSAY

### Instructions For Use

CE 0123

REVISION DATE: 2019-03  
MAK0011-ENG-6

Note Changes Highlighted

REF (18 tests kit) : 11080-018  
(36 tests kit) : 11080-036

#### NAME AND INTENDED USE

The **MP Diagnostics HTLV BLOT 2.4** is a qualitative enzyme immunoassay for the *in vitro* detection of antibodies to HTLV-I and HTLV-II in human serum or plasma. It is intended for use as a more specific supplemental test on human serum or plasma specimens found repeatedly reactive using screening procedures like the Enzyme-Linked Immunosorbent Assays (ELISA).

#### INTRODUCTION

Recent epidemiology studies in the United States and Europe confirm the presence of a mixed prevalence of both HTLV-I and HTLV-II among different high risk populations such as intravenous drug users. Screening tests for HTLV-I/II are widely available. Repeatedly reactive specimens from screening tests require additional and more specific tests to confirm HTLV-I or HTLV-II seropositivity. Such supplemental tests must be capable of identifying antibodies to core (*gag*) and envelope (*env*) proteins of HTLV-I and HTLV-II. Western Blot strips incorporating HTLV-I native viral antigens is one such commonly used supplemental test. However, due to the lack of native envelope antigens on the classical HTLV-I Western Blot, it is often necessary to use radioimmunoprecipitation methods to further confirm for the presence of HTLV-I/II antibodies. Discrimination of HTLV-I and HTLV-II seropositives require supplemental assays (i.e. specific peptide, ELISAs, PCR).

Simple, yet specific and sensitive supplemental serological tests are therefore needed to enable rapid confirmation and differentiation of HTLV-I and HTLV-II seropositive samples.

The **MP Diagnostics HTLV Blot 2.4** has improved sensitivity and specificity for both the confirmation and differentiation of HTLV-I and HTLV-II seroreactivities. This is accomplished by incorporating MTA-1, a unique HTLV-I envelope recombinant protein (rgp46-I), K55, a unique HTLV-II envelope recombinant protein (rgp46-II) and GD21, a common yet specific HTLV-I and HTLV-II epitope envelope recombinant protein (rgp21). Each strip also includes an internal sample addition control to minimize the risk of false negatives due to operational errors.

The **MP Diagnostics HTLV Blot 2.4** is intended as a supplemental antibody assay for characterizing samples found repeatedly reactive by initial HTLV-I/II antibody screening methods. The possible serological profiles defined by the **MP Diagnostics HTLV Blot 2.4** include the following: HTLV Seropositive, HTLV-I Seropositive, HTLV-II Seropositive, Seronegative or Indeterminate.

17. Ensure that automated equipment if used is validated before use.

18. Ensure that the specimens are added away from the strip. Tray can be tilted and specimen added where the buffer is collected at lower end. This prevents dark spot formation due to specimen addition on the strip.

19. Avoid the use of self-defrosting freezers for the storage of reagents and samples.

#### STORAGE

- Store MP Diagnostics HTLV BLOT 2.4 kit and its components at 2-8°C when not in use.
- All test reagents and strips when stored at 2°C to 8°C, are stable until the expiry date given on the kit. Do not freeze reagents.

- Antigen strips**
  - Avoid unnecessary exposure of antigen strips to light.
- Reagents**
  - Store reagents in their original vials or bottles, and they should be closed for storage.
  - Dispense all reagents while cold and return to 2°C to 8°C storage as soon as possible.
  - Precipitates may form when the Substrate is stored at 2°C to 8°C. This will not affect the performance of the kit.

**CAUTION:** Avoid unnecessary exposure of substrate to light.

#### SPECIMEN COLLECTION, TRANSPORT AND STORAGE

Serum or plasma samples collected in EDTA, heparin or sodium citrate may be used. Before storage, ensure that blood clot or citrate cells have been separated by centrifugation.

Samples should be stored at 2°C to 8°C if the test is to be run within 7 days of collection or frozen at -20°C or colder if the test is to be delayed for more than 7 days. Clear, non-hemolyzed samples are preferred. Lipemic, icteric or contaminated (particulate) samples should be filtered (0.45µm) or centrifuged before testing.

Samples can be inactivated but this is not a requirement for optimal test performance.

Inactivate as follows:

- Loosen cap of sample container.
- Heat-inactivate sample at 56°C for 30 minutes in a water bath.
- Allow sample to cool down before retightening cap.
- Sample can be stored frozen until analysis.

Repeated freeze-thawing of sample is not recommended.

#### ADDITIONAL MATERIALS REQUIRED BUT NOT PROVIDED

- Deionized or distilled water
- Disposable gloves
- Rocking platform (designed with a rocking speed of 12 to 16 oscillations per minute and which moves through a 5° to 10° tilt to wash membranes evenly)
- Pipettors and tips of appropriate volume
- Aspirator with sodium hypochlorite trap
- 56°C water bath (optional)
- Sodium hypochlorite for decontamination

#### DESCRIPTION OF SYMBOLS USED

The following are graphical symbols used in or found on **MP Diagnostics** products and packaging. These symbols are the most common ones appearing on medical devices and their packaging. Some of the common symbols are explained in more detail in the European and International Standard EN ISO 15223-1: 2016.

	Use by <i>Synonym for this:</i> Expiry Date		In vitro diagnostic medical device
	Batch Code <i>Synonyms for this are:</i> Lot Number Batch Number		Catalogue Number
	Caution		Authorised Representative in the European Community
	Temperature Limitation		Consult instructions for use
	Manufacturer		Do not reuse
	Contains sufficient for <n> tests		Contents

#### CHEMICAL & BIOLOGICAL PRINCIPLES OF THE PROCEDURE

The nitrocellulose strips are incorporated with HTLV-I viral proteins derived from native inactivated disrupted viral particles and genetically engineered proteins. Individual nitrocellulose strips are incubated with diluted serum or plasma specimens and controls. Specific antibodies to HTLV-I/II, if present in the specimen will bind to the HTLV-I/II proteins on the strips. The strips are washed to remove unbound materials while antibodies that bind specifically to the HTLV proteins can be visualized using a series of reactions with goat anti-human IgG conjugated with alkaline phosphatase and the substrate, BCIP/NBT. This method is sensitive enough to detect marginal amounts of HTLV antibodies in serum or plasma.

1

#### KIT COMPONENTS

Component Description	Quantity Provided
<b>NITROCELLULOSE STRIPS</b> Incorporated with HTLV-I viral lysate, recombinant envelope antigens and a serum addition control (anti-human IgG) band. Keep dry and away from light.	Available in 18 or 36 strips
<b>NON-REACTIVE CONTROL</b> Inactivated normal human serum non-reactive for anti- HCV, anti-HIV-1/2, anti-HTLV-I/II and HBsAg. Contains sodium azide and thimerosal as preservatives.	1 vial (80 µl)
<b>STRONG REACTIVE CONTROL I</b> Inactivated human serum with high titered antibodies to HTLV-I and non-reactive for anti-HCV, anti-HIV-1/2 and HBsAg. Contains sodium azide and thimerosal as preservatives.	1 vial (80 µl)
<b>STRONG REACTIVE CONTROL II</b> Inactivated human serum with high titered antibodies to HTLV-II and non-reactive for anti-HCV, anti-HIV-1/2 and HBsAg. Contains sodium azide and thimerosal as preservative.	1 vial (80 µl)
<b>LYOPHILIZED STOCK BUFFER</b> To be reconstituted in reagent grade water. Tris buffer with heat inactivated animal and non-animal proteins. Contains thimerosal as preservative.	1 or 2 bottles (each to be reconstituted to 100 ml)
<b>WASH BUFFER CONCENTRATE (20x)</b> Tris with Tween-20 and contains thimerosal as preservative.	1 bottle (70 ml)
<b>CONJUGATE</b> Goat anti-human IgG conjugated with alkaline phosphatase.	1 vial (120 µl)

#### Procedure:

- Using forceps, carefully remove required number of STRIPS from the tube and place numbered side up into each well. Include strips for Strong Reactive, Weak Reactive and Non-Reactive controls.
- Add 2 ml of DILUTED WASH BUFFER to each well. **2 ml**
- Incubate the strips for at least 5 minutes at room temperature (25 ± 3°C) on a rocking platform (speed of 12 to 16 oscillations per minute). Remove buffer by aspiration. **5 minutes**
- Add 2 ml of BLOTTING BUFFER to each well. **2 ml**
- Add 20 µl each of patients' sera or controls to appropriate wells. **20 µl**
- Cover the tray with the cover provided and incubate for 1 hour at room temperature (25 ± 3°C) on the rocking platform. **60 minutes**
- Carefully uncover the tray to avoid splashing or mixing of samples . Tilt the tray to aspirate the mixture from the wells. Change aspirator tips between samples to avoid cross-contamination.
- Wash each strip 3 times with 2 ml of DILUTED WASH BUFFER allowing 5 minutes soak on the rocking platform between each wash. **3 x 2 ml**
- Add 2 ml of WORKING CONJUGATE SOLUTION to each well. **2 ml**
- Cover tray and incubate for 1 hour at room temperature (25 ± 3°C) on the rocking platform. **60 minutes**
- Aspirate CONJUGATE from the wells. Wash as in step 8. **3 x 2 ml**
- Add 2 ml of SUBSTRATE SOLUTION to each well. **2 ml**
- Cover tray and incubate for 15 minutes on the rocking platform. **15 minutes**
- Aspirate the SUBSTRATE and rinse the strips at least three times with reagent grade water to stop the reaction. **3 x 2 ml**
- Using forceps, gently remove strips onto paper towels. Cover with paper towels and dry. Alternatively, allow strips to dry in the wells of the tray.
- Mount strips on worksheet (non-absorbent white paper). Do not apply adhesive tape over the developed bands. Observe the bands (See Interpretation of Results) and grade the results. For storage, keep the strips in the dark.

<b>SUBSTRATE</b> Solution of 5-bromo-4-chloro-3-indolyl-phosphate (BCIP) and nitroblue tetrazolium (NBT).	1 bottle (100 ml)
<b>BLOTTING POWDER</b> Non-fat dry milk	10 packets (1g each)
Instructions For Use	1 copy
Protein Finder	1 piece
Forceps	1 piece
Incubation tray*	

Note : Volume of reagents provided are sufficient for 4 runs.

\* Incubation trays provided but packed separately from the kit.

#### WARNINGS AND PRECAUTIONS

- For *in vitro* diagnostic use only.
- For Professional use only.
- Please refer to the product labelling for information on potentially hazardous components.

#### HEALTH AND SAFETY INFORMATION

**CAUTION:** This kit contains materials of human origin. No test method can offer complete assurance that human blood products will not transmit infection.

**HANDLE ASSAY SPECIMENS, STRONG REACTIVE I, STRONG REACTIVE II AND NON-REACTIVE CONTROLS AS POTENTIALLY INFECTIOUS AGENTS.** It is recommended that the components and test specimens be handled using good laboratory working practices. They should be disposed of in accordance with established safety procedures.

The *Strong Reactive Control, Weak Reactive Control and Non-Reactive Control* contain Thimerosal and Sodium azide while *Stock Buffer Concentrate* and *Wash Buffer Concentrate* contain Thimerosal and Conjugate contains Sodium azide. Sodium Azide can react with copper and lead used in some plumbing systems to form explosive salts. The quantities used in this kit are small, nevertheless when disposing of azide-containing materials they should be flushed away with relatively large quantities of water to prevent metal azide buildup in plumbing system.

Pursuant to EC regulation 1272/2008 (CLP), hazardous components are classified and labelled as follows:

Component:	Nitrocellulose strips
<b>Signal Word:</b>	<b>Danger</b>
<b>Pictogram:</b>	
<b>Hazard Statements:</b>	H228 Flammable solid
<b>Precautionary Statements:</b>	P210 Keep away from heat/sparks/open flames/hot surfaces. – No smoking. P280 Wear protective gloves/protective clothing/eye protection/face protection.

SUMMARY OF ASSAY PROTOCOLS			
Reagents	Qty	Duration	
Nitrocellulose strip	1	-	
Wash Buffer	2 ml	5 mins	
Blotting Buffer	2 ml	-	
Specimen	20 µl	60 mins	
Wash Buffer	3 x 2 ml	3 x 5 mins	
Conjugate	2 ml	60 mins	
Wash Buffer	3 x 2 ml	3 x 5 mins	
Substrate (Ready to use)	2 ml	15 mins	
Distilled Water	3 x 2 ml	-	

Reagents	NUMBER OF STRIPS TO BE USED							
	3	6	9	15	20	27	36	
1X Wash Buffer (ml)	60	100	140	240	300	400	520	
1X Blotting Buffer (ml)	20	40	60	80	100	120	160	
Conjugate (µl)	11	17	23	35	45	59	77	
Substrate (ml)	11	17	23	35	45	59	77	
Blotting Powder (g)	1	2	3	4	5	6	8	

#### QUALITY CONTROL

We recommend that the Non-Reactive Control and both Strong Reactive Controls be run with every assay regardless of the number of samples tested. In order for the results obtained from any assay to be considered valid, the following conditions must be met:

- NON-REACTIVE CONTROL**  
No HTLV-I/II viral specific bands, rgp46-I, rgp46-II or GD21 should be observed on the Non-Reactive control strip. The serum control (anti-human IgG) band should be visible.
- STRONG REACTIVE CONTROL I**  
The relevant HTLV bands that must be present are p19, p24, rgp46-I and GD21. The sample control (anti-human IgG) band should be visible.  
**Note:** Although uncommon, a gp46 viral band may be present. If present, it appears as a diffuse band. Because of the rarity of gp46 and misreading of viral bands in this molecular weight range, viral gp46 is not used as part of the assay's interpretative criteria.
- STRONG REACTIVE CONTROL II**  
The serum control band and all relevant HTLV-I/II molecular weight bands must be evident . The relevant HTLV II bands that must be present are p24, GD21 and rgp46-II. The serum control (anti-human IgG) band should be visible.

<b>Supplemental Statements:</b>	EUH210 Safety Data Sheet is available on request
<b>Contains:</b>	100% Nitrocellulose

<b>Component:</b>	<b>STOCK BUFFER CONCENTRATE (10x)</b> <b>WASH BUFFER CONCENTRATE (20x)</b>
<b>Signal Word:</b>	Warning
<b>Pictogram:</b>	
<b>Hazard Statements:</b>	H373 May cause damage to organs through prolonged or repeated exposure
<b>Precautionary Statements:</b>	P260 Do not breathe dust/fume/gas/mist/vapours/spray. P501 Dispose of contents/container in accordance with local/regional/national/international regulations.
<b>Supplemental Statements:</b>	EUH210 Safety Data Sheet is available on request
<b>Contains:</b>	0.1% Thimerosal

- Avoid Microbial contamination of reagents when opening and removing aliquots from the original vials or bottles.
- Do not pipette by mouth.
- Handle test specimens, nitrocellulose strips, Strong Reactive I, Strong Reactive II and Non-Reactive Controls as potentially infectious agents.
- Wear laboratory coats and disposable gloves while performing the assay. Discard gloves in bio-hazard waste-bags. Wash hands thoroughly afterwards.
- It is highly recommended that this assay be performed in a biohazard cabinet.
- Keep materials away from food and drink.
- In case of accident or contact with eyes, rinse immediately with plenty of water and seek medical advice.
- Consult a physician immediately in the event that contaminated materials are ingested or come in contact with open lacerations, or other breaks in the skin.
- Wipe spills of potentially infectious materials immediately with absorbent paper and swab the contaminated area with 1% sodium hypochlorite solution before work is resumed. Sodium hypochlorite should not be used on acid containing spills unless the area is wiped dry with absorbent paper first. Material used (including disposable gloves) should be disposed of as potentially biohazardous material. Do not autoclave material containing sodium hypochlorite.
- Autoclave all used and contaminated materials at 121°C at 15 p.s.i. for 30 minutes before disposal. Alternatively, decontaminate materials in 5% sodium hypochlorite solution for 30-60 minutes before disposal in biohazard waste-bags.

#### INTERPRETATION OF RESULTS

The serum control band serves as a check for serum addition in the assay. Absence of this band indicates that no test serum or conjugate or substrate has been dispensed onto the test strip or other operational errors.

Locate and identify bands on the strips run with Strong Reactive Controls. These strips are then used to identify bands present on strips used with test specimens.

PATTERN	INTERPRETATION
1. No reactivity to HTLV specific proteins	SERONEGATIVE
2. Reactivity to GAG (p19 with or without p24) and two ENV (GD21 and rgp46-I)	HTLV-I SEROPOSITIVE
3. Reactivity to GAG (p24 with or without p19) and two ENV (GD21 and rgp46-II)	HTLV-II SEROPOSITIVE
4. Reactivity to GAG (p19 and p24) and ENV (GD21) <i>-HTLV-I SEROPOSITIVE indicated if p19 ≥ p24</i> <i>-HTLV-II SEROPOSITIVE indicated if p19 &lt; p24</i>	HTLV SEROPOSITIVE*
5. HTLV specific bands detected but does not meet criteria for HTLV-I, HTLV-II or HTLV Seropositive. However, the following indeterminate banding patterns can be interpreted as <i>SERONEGATIVE</i> :	INDETERMINATE**

- HTLV-I GAG Indeterminate Western blot patterns (HGIP) Presence of p19, p26, p28, p32, p36, p53 but absence of p24 and any ENV proteins*
- Any combination of GAG proteins (p19, p26, p28, p32, p36, p53) but absence of p24 and any ENV proteins*
- Any single GAG proteins (p19, p24, p26, p28, p32, p36, p53)*

Non-typeable HTLV seropositive can be further resolved by using *Viktor et al's* algorithm in the absence of rgp46-I and rgp46-II. This algorithm which uses the relative reactivity of the two serotypes, <sup>7,11,12,13,14</sup>

Indeterminate interpretation is based on WHO's 1990 guideline.<sup>15</sup> However, various studies suggested that certain indeterminate banding patterns (as listed) can be interpreted as seronegative especially with healthy blood donors.<sup>16-26</sup> For example, a study involving 37,724 healthy blood donors, confirmed that HGIP can be safely interpreted as seronegative.<sup>26</sup> However, caution should be exercised when indeterminate patterns are obtained with IVD users or blood donors from endemic areas, and neurological disease patients.<sup>26,27</sup>

11. Decontaminate all used chemicals and reagents by adding sufficient volume of sodium hypochlorite to make a final concentration of at least 1%. Leave for 30 minutes to ensure effective decontamination.

12. We do not recommend re-use of incubation trays.

#### ANALYTICAL PRECAUTIONS

- Optimal assay performance requires **STRICT ADHERENCE** to the assay procedure described in this Instruction Manual. Deviations from the procedure may lead to aberrant results.
- DO NOT MODIFY OR SUBSTITUTE REAGENTS FROM ONE KIT LOT TO ANOTHER.** Controls, conjugate and Western Blot strips are matched for optimal performance. Use only the reagents supplied with the kit.
- Do not use kit components beyond the expiry date printed on the kit box.
- Avoid microbial contamination of the reagents, when opening and removing aliquots from the original vials or bottles. As this will prematurely reduce the shelf life of the kits and give erroneous results. Use aseptic techniques including pipettes or disposable pipette tips when drawing aliquots from vials.
- The kit controls should be assayed concurrently with patients' samples for each test run.
- Use a new pipette tip for each specimen aliquot to prevent cross contamination.
- For best results dispense all reagents while cold and return to 2°C to 8°C storage as soon as possible.
- It is recommended that glassware to be used with the reagents should be washed with 2M hydrochloric acid and rinsed thoroughly with distilled or deionised water prior to use.
- Use only reagent grade quality, deionised or distilled water to dilute reagents.
- All reagents must be mixed well before use.
- Working Conjugate solution, Diluted Wash Buffer and Blotting Buffer should be **prepared fresh prior to use.**
- The Working Conjugate solution should be prepared using a polypropylene container or beaker.
- Do not expose reagents or perform test in an area containing a high level of chemical disinfectant fumes (e.g. hypochlorite fumes) during storage or during incubation steps. Contact inhibits colour reaction. Also do not expose reagents to strong light.
- The assay should preferably be performed at room temperature (25°C ± 3°C).
- Make sure that the test strips are laid with the numbers on the strips facing upwards.
- For Western Blot Assay, it is important to use a rocking platform shaker and not a rotary shaker. Otherwise, performance of the kit will be compromised. The recommended speed and tilt angle of the shaker are 12 to 16 cycles per minute, and 5 to 10 degrees, respectively.

3

#### IDENTIFICATION OF BANDS

The Protein Finder (Figure 1) provided in the kit is used to locate and identify bands on the strips run with Strong Reactive Control I and Strong Reactive Control II. These control strips are then used to identify bands present on strips used with test specimens. Each Protein Finder is lot specific; only the Protein Finder that comes with the kit should be used to locate and identify bands.

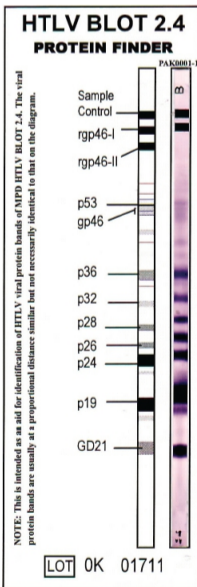


Figure 1: Example of a Protein Finder

#### LIMITATIONS OF THE METHOD

Serum from individuals with dual infections although rare, may occur and can also be differentiated based on the above criteria. Banding patterns of such specimens will indicate HTLV-I and HTLV-II positive. Available data demonstrates that the seroreactivities to rgp46-I and rgp46-II are specific for HTLV-I and HTLV-II respectively. Therefore sera reactive to rgp46-I, rgp46-II, GD21, p19 and p24 will provide a dual infection classification.

Optimal assay performance requires the strict adherence to the assay procedure described. Deviation from the procedure may lead to aberrant results.

ANEGATIVE result does not exclude the possibility of exposure to or infection with HTLV-I or HTLV-II. INDETERMINATE blots should not be used as the basis for diagnosis of HTLV-I/II infection.

It is also reported that both p19 or p24 seroreactivities have been observed in uninfected low risk populations although p24 indeterminants are relatively rare.

The sensitivity of rgp46-I has been reported to be 95% in France, 100% of PCR confirmed samples in Jamaica and the United States, and 98% of HTLV-I seropositive blood donors. The sensitivity of rgp46-II has been shown to be more than 98% among PCR confirmed samples from United States.

4

5

6



The overall sensitivity of each type specification, rgp46-I and rgp46-II, is estimated to be greater than 97%. The small percentage of HTLV-I and HTLV-II samples that are not reactive with either rgp46-I or rgp46-II are reactive with at least GD21 and one or more GAG bands, p19, or p24 meeting the criteria of either HTLV seropositive (Pattern 4) or Indeterminate (Pattern 5). There were no false negative interpretations reported.

Supplemental test such as PCR (HTLV-I and HTLV-II) may be useful in the discrimination of HTLV seropositive samples that cannot be identified as either HTLV-I or HTLV-II with the MP Diagnostics HTLV Blot 2.4 (i.e Pattern 4).

### SPECIFIC PERFORMANCE CHARACTERISTICS

The performance of MP Diagnostics HTLV Blot 2.4 for the detection of antibodies to HTLV-I and HTLV-II was evaluated using HTLV-I/II seropositive and seronegative specimens and was compared with two line immunoassays which incorporate HTLV I and HTLV II antigens (recombinant proteins or peptides).

### Sensitivity

Specimens which are established to be positive for HTLV I or / and HTLV II antibodies by commercial ELISAs were used to determine the sensitivity of MP Diagnostics HTLV Blot 2.4.

A. Comparison to Line Immunoassay 1  
Blot result comparing to MP Diagnostics HTLV Blot 2.4 and Line Immunoassay 1 (LI 1) for positive samples purchased from Boston Biomedical, Inc., USA (BBI), and ProMedDx were as follows:

Method	Line Immunoassay 1			Total
	NEG / IND	POS	0	
MP Diagnostics HTLV BLOT 2.4	NEG / IND	3*	0	3
	POS	0	102	102
	Total	3	102	105

\* MP Diagnostics HTLV Blot 2.4 gave 2 indeterminate and 1 negative result which was also detected negative by Line Immunoassay 1. Line Immunoassay 1 gave 3 negative results.

The two blots gave the following discriminations for the 102 HTLV positive samples:

Method	Interpretation				Total
	HTLV I	HTLV II	HTLV I & HTLV II**	Non-typeable***	
MP Diagnostics HTLV BLOT 2.4	45	53	4	0	102
LI 1	48	51	0	3	102

\*\* Both HTLV I and HTLV II specific markers appeared, indicating co-infection.

\*\*\* Unable to type HTLV strains because of the absence of specific markers.

Both MP Diagnostics HTLV Blot 2.4 and LI 1 gave similar results. The few discordant results are due to different antigens immobilized on the blots and the different methods used.

MP Diagnostics HTLV Blot 2.4 showed a sensitivity of 97.1% which was equivalent to that obtained with Line Immunoassay 1.

### B. Comparison to Line Immunoassay 2

The French Society of Blood Transfusion Anti-HTLV-I and II Performance Panel, SFTS-94 consisting of 26 HTLV-1 and 6 HTLV-II samples were studied. Results of MP Diagnostics HTLV Blot 2.4 on this panel were compared to Line Immunoassay 2 (LI 2) as follows:

Method	Interpretation				Total
	HTLV I	HTLV II	Non-typeable	False NEG	
MP Diagnostics HTLV BLOT 2.4	26	6	0	0	32
LI 1	21	6	4	1	32

MP Diagnostics HTLV Blot 2.4 correctly identifies HTLV positive samples, giving a sensitivity of >99.9% in this panel. Using the same panel, the comparative kit (LI 2) gave a sensitivity of 96.9%.

### Specificity

A total of 200 blood donor samples were tested resulting in a specificity of 92.5%. 15 samples were indeterminate and there were no false positive results.

If 150 clinical specimens, 50 pregnancy specimens, 50 potentially interfering specimens (10 each of icteric, haemolysed, triglyceride, lipemic, total protein specimens), and 73 potentially cross-reactive specimens (TB, *Helicobacter pylori*, HEV, Dengue, HBV, HCV, HIV-1, HIV-2), are included, the overall specificity was 89.2% (461/517). 56 samples were indeterminate and there were no false positive results. 6 samples were true positives confirmed by another confirmatory test.

### LIMITED EXPRESSED WARRANTY DISCLAIMER

The manufacturer makes no expressed warranty other than that the test kit will function as an *in-vitro* diagnostic assay within the specifications and limitations described in the product Instruction Manual when used in accordance with the instructions contained therein. The manufacturer disclaims any warranty expressed or implied, including such expressed or implied warranty with respect to merchantability, fitness for use or implied utility for any other purposes. The manufacturer is limited to either replacement of the product or refund of the purchase price of the product. The manufacturer shall not be liable to the purchaser or third parties for any damage, injury or economic loss however caused by the product in the use or in the application thereof.

### TECHNICAL PROBLEMS / COMPLAINTS

Should there be a technical problem / complaint, please do the following :

- Note the kit lot number and the expiry date.
- Retain the kits and the results that were obtained.
- Contact the nearest MP Biomedicals office or your local distributor.

### BIBLIOGRAPHY

- Towbin H., Staehlin T. and Gordon J. Electrophoretic transfer of proteins from polyacrylamide gels to nitrocellulose sheets: procedure and some applications. Proc. Natl. Acad. Sci. U.S.A. 1976; 76: 4350-4354.

- Poiesz BJ., Ruscetti FW., Gazdar AF., Bonn PA., Minna JD. And Gallo RC. Detection and isolation of type C retrovirus particles from fresh and cultured lymphocytes of a patient with cutaneous T-cell lymphoma. Proc. Natl. Acad. Sci. U.S.A. 1980; 77(12): 7415-7419.
- Kalyanaraman VS., Sarngadharan MG., Robert-Guroff M., Miyoshi I., Blayney D., Golde and Gallo RC. A new subtype of human T-cell leukemia virus (HTLV-II) associated with a T-cell variant of hairy cell leukemia. Science 1982; 218: 571-573.
- William AE., Fang CT., Slamon DJ. et al. Seroprevalence and epidemiological correlates of HTLV-I infection in U.S. blood donors. Science 1988; 240: 643-646.
- Lee H., Swanson P., Shorty VS., Zack JA., Roseblatt JD. and Chen ISY. High rate of HTLV-II infection in seropositive IV drug abusers in New Orleans. Science 1989; 244: 471-475.
- Lipka JJ., Bui K., Reyes GR, Moeckli R., Wiktor SZ., Blattner WA., Murphy EL., Hanson CV., Shaw GM., Shinsky JJ. and Fong SKH. Determination of a unique immunodominant epitope of HTLV-I. Infect Dis 1990; 162: 353-357
- Wiktor SZ., Alexandra SS., Shaw GM. et al. Distinguishing between HTLV-I and HTLV-II by Western Blot. Lancet 1990; 335: 1533.
- Samuel KP., Lautenberger JA., Jorcyk CL., Josephs S., Wong Staal F. and Papas TS. Diagnostic potential for human malignancies of bacterially produced HTLV-I envelope protein. Science 1984; 226: 1094-1097.
- Hadlock KG., Goh CJ., Bradshaw PA., Perkins S., Lo J., Habbaz RK., Kaplan J. and Fong SKH. Delineation of an immunodominant and highly HTLV specific epitope within the HTLV-I transmembrane glycoprotein. Blood 1995; 68(4): 1392-1399.
- Varma M., Rudolph D., Knuchel M., Switzer W., Hadlock KG., Velligan M., Chan L., Fong SKH., Lal RB. Enhanced specificity of truncated transmembrane protein for serologic confirmation of HTLV-I and HTLV-II infection by Western Blot assay containing recombinant envelope glycoproteins. J. Clin. Micro. 1995; 33(12): 3239-3244.
- Lillehoj EP, Alexander SS, Dubrule C.J., Wiktor S., Adams R., Thi, A. Manns CC., and Blattner WA. Development and evaluation of a human T-Cell leukemia virus type I serologic confirmatory assay incorporating a recombinant envelope polypeptide. J. Clin. Microbiol. 1990; 28: 2653-2658.
- Lal RB., Brodine SK., Coligan JE., and Roberts CR. Differential antibody responsiveness to p19 gag results in serological discrimination between human T-lymphotropic virus type I and type II. J. Med. Virol. 1991; 1: 232-236.
- Hjelle B., Cyrus S., Swenson S., and Mills R. Serologic distinction between human T-lymphotropic virus (HTLV) type I and HTLV type II. Transfusion 1991; 31: 731-736.
- Madeleine, MM., Wiktor SZ., Goedert JI., Manns A., Levine PH., Biggar RJ., Blattner WA. HTLV-I and HTLV-II worldwide distribution: reanalysis of 4,832 immunoblot results. Inte. J. Cancer 1993; 54(2): 255-260.

- World Health Organization's Global Programme on AIDS. WHO Global Programme on AIDS Information Update. Virus Information Exchange Newsletter 1990; 7(2): 54-55.
- Lal, RB., Rudolph DL., Coligan JE., Brodine SK., and Roberts CR. Failure to detect evidence of human T-lymphotropic virus (HTLV) type I and type II in blood donors with isolated gag antibodies to HTLV-I/II. Blood 1992; 80: 544-550.
- Khabbaz, RF., Heineke W., Grindon A., Hartley TM., Shulman G., and Kaplan J. Indeterminate HTLV serologic results in U.S. blood donors: Are they due o HTLV-I or HTLV-II? J. Acquir. Immune Defic. Syndr. 1992; 5: 400-404.
- Lipka, JJ., Young KK., Kwok SY., Reyes GR., Shinsky JJ, and Fong SK. Significance of human T-lymphotropic virus type I indeterminate serological findings among healthy individuals. Vox Sang. 1991; 61: 171-176.
- Zrein M., Louwagie J., Boeykens H., Govers L., Hendicx G., Bosman F., Sablon E., Demarquilly C., Boniface M., and Saman E. Assessment of a new immunoassay for serological confirmation and discrimination of human T-cell lymphotropic virus infections. Clin. Diag. Lab. Immunol. 1998; 5: 45-49.
- Witt DJ., Kuramoto K., Kemper M., and Holland P. Utility of prospective study of donors deferred as HTLV indeterminate. Vox Sang. 2000; 78:130-131.
- Hayes C.G., Burans JP., and Oberst RB. Antibodies to Human T Lymphotropic virus Type I in a population from the Philippines: Evidence for cross-reactivity with *Plasmodium falciparum*. The J. Infect. Dis. 1990; 163: 257-262.
- Gallo D., Diggs JL., and Hanson CV. Evaluation of two commercial Human T-Cell Lymphotropic Virus Western blot (Immunoblot) kits with problem specimens. J. Clin. Microbiol. 1994; 32: 2046-2049.
- Garin B., Gosselin S., de The G., and Gessain A. HTLV-I/II infection in a high viral endemic area of Zaire, Central Africa: Comparative evaluation of serology, PCR, and significance of indeterminate Western blot pattern. J. Med. Virol. 1994; 44: 104-109.
- Fujiyama C., Fujiyoshi T., Matsumoto D., Yashiki S., Tamashiro H., and Sonoda S. Re-evaluation of anti-HTLV-I Western blot assay using HTLV-I and HTLV-II serum panels. Clin. & Diag. Virol. 1995; 4: 149-161.
- Rouet F., Meertens L., Courouble G., Herrmann-Storck C., Pabingui R., Chanceler B., Abid A., Strobel M., Mauciere P., and Gessain A. Serological, epidemiological, and molecular differences between human T-cell lymphotropic virus type I - seropositive healthy carriers and persons with HTLV-I gag indeterminate Western blot patterns from the Caribbean. J. Clin. Microbiol. 2001; 39: 1247-1253
- Cesaire R., Bera O., Maier H., Lezin A., Martial J., Ouka M., Kerob-Bauchet B., Ould Amar AK., and Vernant JC. Seroindefinite patterns and seroconversions to human T-lymphotropic virus type I positivity in blood donors from Martinique, French West Indies. Transfusion 1999; 39: 1145-1149.

- Soldan SS., Graf MD., Waziri A., Flerlage AN., Robinson SM., Kawaninshi T, Leist TP., Lehky TJ., Levin MC., and Jacobson S. HTLV-I/II seroindefinite western blot reactivity in a cohort of patients with neurological disease. J. Infect. Dis. 1999; 180: 685-694.



### MP Biomedicals Asia Pacific Pte. Ltd.

2 Pioneer Place  
Singapore 627885  
Tel No. : + 65 6775 0008  
Fax No. : + 65 6774 6146  
Email : enquiry\_ap@mpbio.com



### MP Biomedicals Germany GmbH

Thüringer Straße 15  
37269 Eschwege  
Germany  
Tel No. : +49 5651 921 204  
Fax No. : +49 5651 921 181  
Email : diagnostics@mpbio.com


### Regional Office:

#### MP Biomedicals Germany GmbH

Thüringer Straße 15  
37269 Eschwege  
Germany  
Tel No. : +49 5651 921 204  
Fax No. : +49 5651 921 181  
Email : diagnostics@mpbio.com

- \* US Patent: 5,066,579 ; 5,614,366 ; 5,763,572 ; 5,814,441 ; 5,871,933 ; 5,643,714
- \* Australian Patent: 613350 ; 667189 ; 690540
- \* Canadian Patent: 1337799
- \* European Patent: 0395634
- \* Japanese Patent: 2559482

FIGURE 2

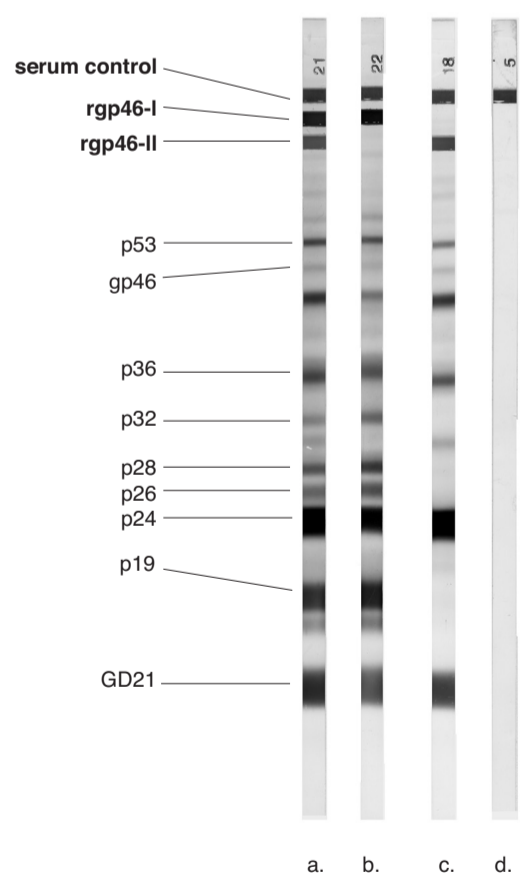

Viral specific bands as visualized with:  
a. A HTLV-I/II dual infection serum.  
b. Strong Reactive Control I. (Reactive for HTLV-I only)  
c. Strong Reactive Control II. (Reactive for HTLV-II only)  
d. Non-reactive Control.

### TROUBLE SHOOTING CHART

